


# DEVICE CONNECTION CABLE TYPE: H1

## PHYSICAL CONNECTIONS

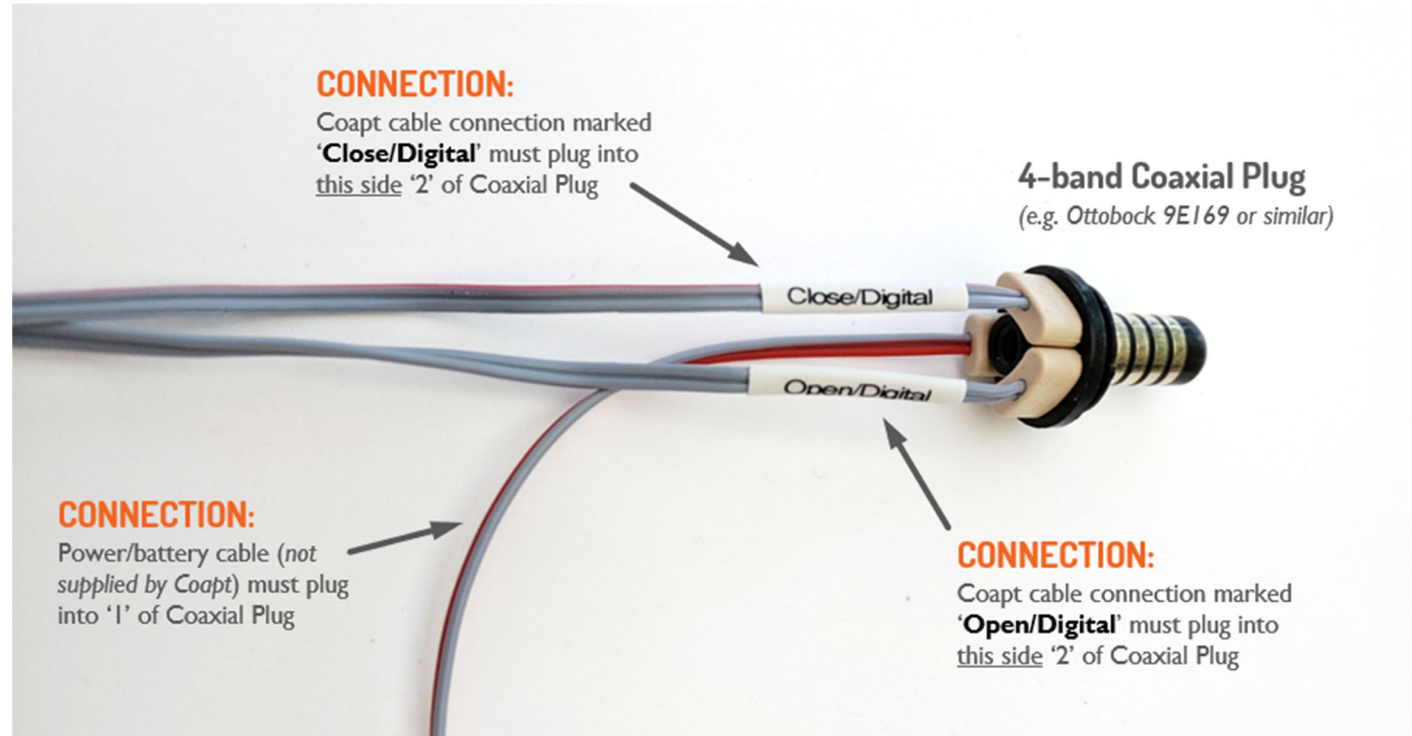

## SOFTWARE SETTINGS

### I-LIMB SETTINGS:

For general i-Limb Digital operation via Coapt, most settings should be set to defaults in the i-Limb app

For proper operation of Gesture Control via Coapt, ensure '**CC**' is selected as its trigger in the i-Limb app

