


# DEVICE CONNECTION CABLE TYPE: H2

## PHYSICAL CONNECTIONS

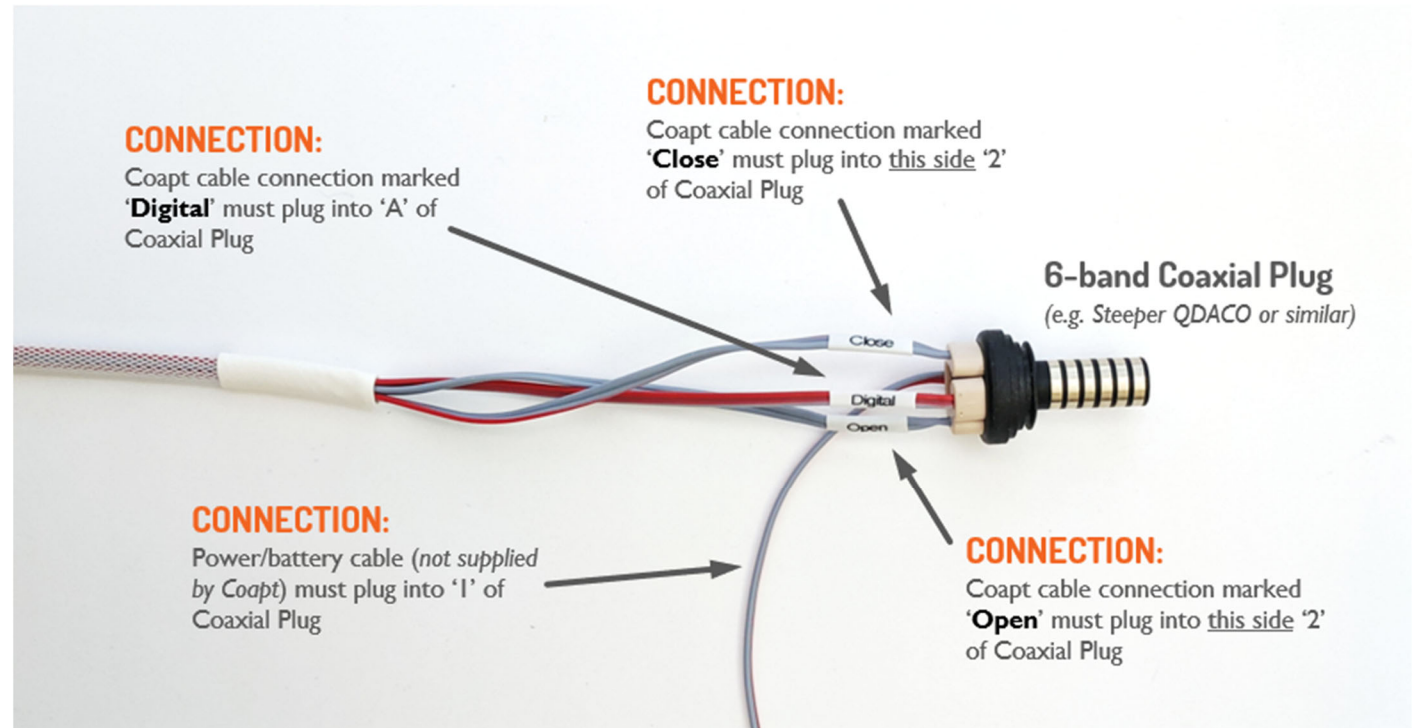

## SOFTWARE SETTINGS

### TASKA HAND SETTINGS:

For digital TASKA hand operation via Coapt, TASKA settings will automatically be set upon each power-on

### BEBIONIC HAND SETTINGS:

For digital bebionic hand operation via Coapt, refer to settings shown in the on-screen guide available at "Connection Guide" in the Coapt Complete ControlRoom Gen2 user interface application