


DEVICE CONNECTION CABLE TYPE: 14

PHYSICAL CONNECTIONS

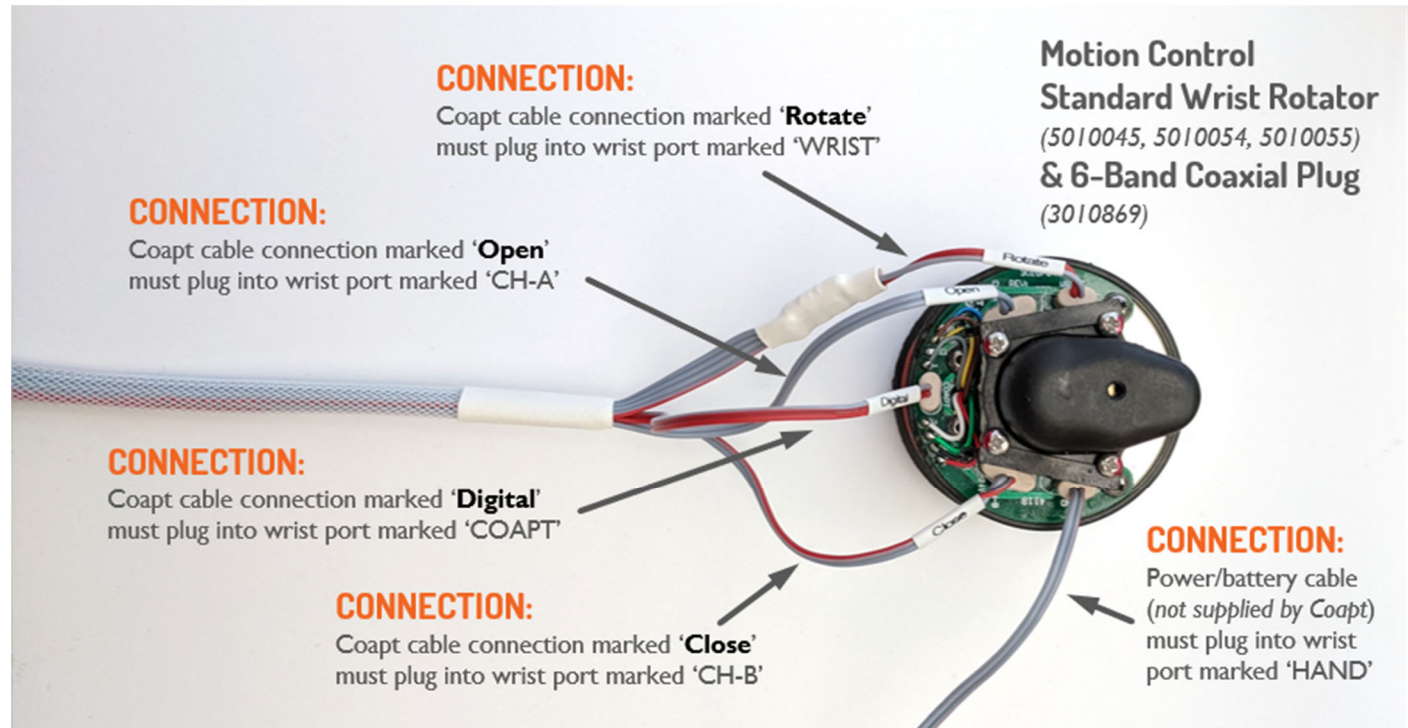

SOFTWARE SETTINGS

WRIST SETTINGS:

No manual settings necessary for the Motion Control Standard Wrist Rotator & 6-Band Coaxial Plug

TASKA HAND SETTINGS:

For digital TASKA hand operation via Coapt, TASKA settings will automatically be set upon each power-on

BEBIONIC HAND SETTINGS:

For digital bebionic hand operation via Coapt, refer to settings shown in the on-screen guide available at "Connection Guide" in the Coapt Complete ControlRoom Gen2 user interface application.